

Thermogravimetric analysis 400°C

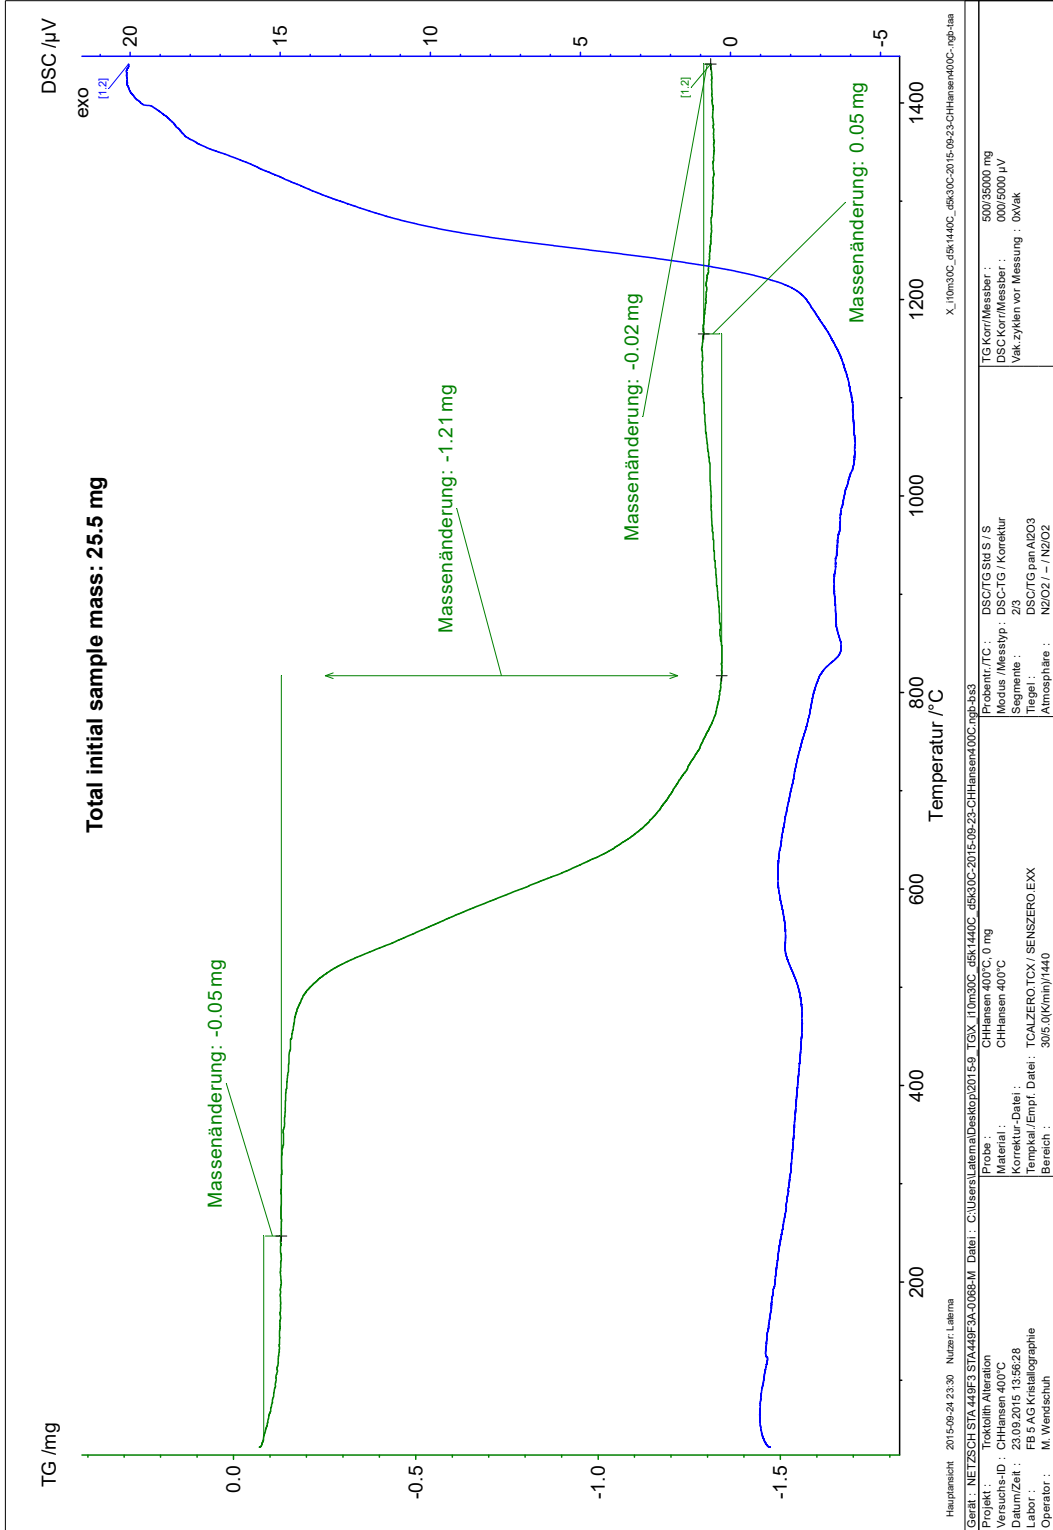


FIGURE S3-2. Evaluated spectrum of thermogravimetric measurement for 400°C.